
**Collection precautions:**

**Do NOT eat, drink, smoke or chew gum for 30 minutes before giving your sample.**

**Do NOT remove the plastic film from the funnel lid.**

**Contents:** Kit contains stabilizing liquid.

**Warnings and precautions:**

Wash with water if stabilizing liquid comes in contact with eyes or skin. Do NOT ingest. See MSDS at [www.dnagenotek.com](http://www.dnagenotek.com).










Small cap may pose a choking hazard.

**Storage:** 15°C / 30°C

**Summary and explanation of the kit:**

OMNigene-ORAL is a collection kit that provides the materials and instructions for collecting, stabilizing and maintaining during transport saliva specimens suspected of containing SARS-CoV-2 ribonucleic acid (RNA).

**Label legend:**

	Consult package insert
	Collect sample by (Use by)
	In vitro diagnostic medical device
	Catalog number
	Caution, consult instructions for use
	Storage instructions
	Manufacturer
	Lot number
	For Prescription Use Only


*Collected specimen is potentially infectious and should be handled with appropriate biosafety practices.*

*Ship in accordance to applicable regulations covering transport of biological specimens.*


For donor collection instructions in other languages, see [www.dnagenotek.com](http://www.dnagenotek.com)

**USER INSTRUCTIONS**


**Most people take between 2 and 5 minutes to deliver a sample following steps 1 to 5.**




- 1** Spit into funnel until the amount of liquid (not bubbles) reaches the fill line shown in picture #1.




- 2** Hold the tube upright with one hand. Close the funnel lid with the other hand (as shown) by firmly pushing the lid until you hear a loud click. The liquid in the lid will be released into the tube to mix with the sample. Make sure that the lid is closed tightly.



- 3** Hold the tube upright. Unscrew the funnel from the tube.



- 4** Use the small cap to close the tube tightly.



- 5** Shake the capped tube for 5 seconds. Discard or recycle the funnel.

For IVD, Rx and For Use Under Emergency Use Authorization.

This sample collection device has not been FDA cleared or approved.

This sample collection device has been authorized by FDA under an EUA.

This sample collection device has been authorized only to collect, stabilize, and maintain during transport, saliva specimens suspected of containing SARS-CoV-2 ribonucleic acid (RNA), not for any other viruses or pathogens.

This sample collection device is only authorized for the duration of the declaration that circumstances exist justifying the authorization of emergency use of medical devices during the COVID-19 outbreak under Section 564(b)(1) of the Federal Food, Drug, and Cosmetic Act, 21 U.S.C. § 360bbb-3(b)(1), unless the authorization is terminated or revoked sooner.

**DNAGENOTEK™**


Made in Canada ■ DNA Genotek Inc.  
3000 - 500 Palladium Drive  
Ottawa, ON, Canada K2V 1C2

*Superior samples • Proven performance*

Toll-free (North America): 1.866.813.6354  
Tel: +1.613.723.5757 • Fax: +1.613.723.5057  
[info@dnagenotek.com](mailto:info@dnagenotek.com) • [www.dnagenotek.com](http://www.dnagenotek.com)

™DNA Genotek is a trademark and \*OMNigene is a registered trademark of DNA Genotek Inc. Some DNA Genotek products may not be available in all geographic regions, contact your sales representative for details. All DNA Genotek protocols, white papers and application notes, are available in the support section of our website at [www.dnagenotek.com](http://www.dnagenotek.com).

Patent ([www.dnagenotek.com/legalnotices](http://www.dnagenotek.com/legalnotices))  
© 2020 DNA Genotek Inc., a subsidiary of OraSure Technologies, Inc., all rights reserved.  
PD-PR-01058 Issue 1/2020-10

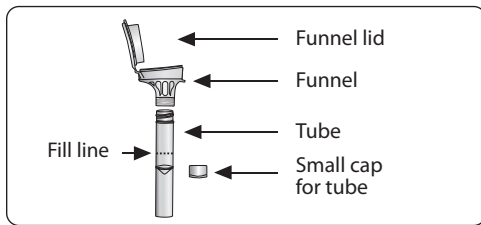
**Collection precautions:**

**Do NOT eat, drink, smoke or chew gum for 30 minutes before giving your sample.**

**Do NOT remove the plastic film from the funnel lid.**

**Contents:** Kit contains stabilizing liquid.

**Warnings and precautions:**

Wash with water if stabilizing liquid comes in contact with eyes or skin. Do NOT ingest. See MSDS at [www.dnagenotek.com](http://www.dnagenotek.com).












Small cap may pose a choking hazard.

**Storage:** 15°C / 30°C

**Summary and explanation of the kit:**

OMNigene-ORAL is a collection kit that provides the materials and instructions for collecting, stabilizing and maintaining during transport saliva specimens suspected of containing SARS-CoV-2 ribonucleic acid (RNA).

**Label legend:**

	Collect sample by (Use by)
	In vitro diagnostic medical device
	Catalog number
	CE Marking
	Consult package insert
	Caution, consult instructions for use
	15°C / 30°C Storage instructions
	Manufacturer
	Authorized Representative
	Lot number
	For Prescription Use Only


*Collected specimen is potentially infectious and should be handled with appropriate biosafety practices.*

*Ship in accordance to applicable regulations covering transport of biological specimens.*


For donor collection instructions in other languages, see [www.dnagenotek.com](http://www.dnagenotek.com)

**USER INSTRUCTIONS**


**Most people take between 2 and 5 minutes to deliver a sample following steps 1 to 5.**




- 1** Spit into funnel until the amount of liquid (not bubbles) reaches the fill line shown in picture #1.




- 2** Hold the tube upright with one hand. Close the funnel lid with the other hand (as shown) by firmly pushing the lid until you hear a loud click. The liquid in the lid will be released into the tube to mix with the sample. Make sure that the lid is closed tightly.



- 3** Hold the tube upright. Unscrew the funnel from the tube.



- 4** Use the small cap to close the tube tightly.



- 5** Shake the capped tube for 5 seconds. Discard or recycle the funnel.



**For IVD, Rx and For Use Under Emergency Use Authorization.**

This sample collection device has not been FDA cleared or approved.

This sample collection device has been authorized by FDA under an EUA.

This sample collection device has been authorized only to collect, stabilize, and maintain during transport, saliva specimens suspected of containing SARS-CoV-2 ribonucleic acid (RNA), not for any other viruses or pathogens.

This sample collection device is only authorized for the duration of the declaration that circumstances exist justifying the authorization of emergency use of medical devices during the COVID-19 outbreak under Section 564(b)(1) of the Federal Food, Drug, and Cosmetic Act, 21 U.S.C. § 360bbb-3(b)(1), unless the authorization is terminated or revoked sooner.

**DNAGENOTEK™**

Made in Canada ■ DNA Genotek Inc.  
3000 - 500 Palladium Drive  
Ottawa, ON, Canada K2V 1C2

*Superior samples • Proven performance*

Toll-free (North America): 1.866.813.6354  
Tel: +1.613.723.5757 • Fax: +1.613.723.5057  
info@dnagenotek.com • www.dnagenotek.com



Emergo Europe, Prinsessegracht 20, 2514 AP The Hague, The Netherlands

™DNA Genotek is a trademark and \*OMNigene is a registered trademark of DNA Genotek Inc. Some DNA Genotek products may not be available in all geographic regions, contact your sales representative for details. All DNA Genotek protocols, white papers and application notes, are available in the support section of our website at [www.dnagenotek.com](http://www.dnagenotek.com).

Patent ([www.dnagenotek.com/legalnotices](http://www.dnagenotek.com/legalnotices))  
© 2020 DNA Genotek Inc., a subsidiary of OraSure Technologies, Inc., all rights reserved.  
PD-PR-01059 Issue 1/2020-10