



January 21, 2021

E


Dear Iuymfu,

This is the Kaiser Permanente Saliva Home Collection Kit that you requested. This test will ask you to collect a sample of your saliva. Test results are usually available on kp.org within 48 hours of when we receive your sample.

Please return the sample back to us using the pre-paid package enclosed following the shipping options on the bottom of this page. **Please return sample back on the same day it was collected. For people 18 years old and older.**

The Kaiser Permanente Saliva Home Collection Kit contents include:

- ✓ Corrugated box
- ✓ Saliva collection device with collection instructions
- ✓ Personalized patient letter with shipping instructions and label
- ✓ Biohazard bag with absorbent tissue
- ✓ Return shipping bag

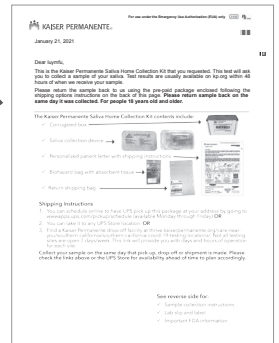

Shipping Instructions


1. You can schedule online to have UPS pick up this package at your address by going to wwwapps.ups.com/pickup/schedule (Monday through Friday) **OR**
2. You can take it to any UPS Store location Monday through Friday (go to www.ups.com/dropoff to learn more; be sure to drop off your completed kit before the latest 'Air' drop-off time) **OR**
3. Find a Kaiser Permanente drop-off facility at thrive.kaiserpermanente.org/care-near-you/southern-california/southern-california-covid-19-testing-locations/. Not all testing sites are open 7 days/week. This link will provide you with days and hours of operation for each site.

Collect your sample (Monday through Friday) on the same day that pick-up, drop-off or shipment is made. Please check the links above ahead of time to plan accordingly.

See reverse side for:

- ✓ Sample collection instructions
- ✓ Lab slip and label
- ✓ Important FDA information

Wash hands prior to sample collection. **Do not eat, drink, smoke or chew gum for 30 minutes before providing the saliva sample.** Do not ingest the liquid in the collection device. Wash with water if liquid solution comes in contact with eyes or skin. Follow all instructions provided in the collection device for sample collection. Not following the instructions exactly can lead to incorrect results.

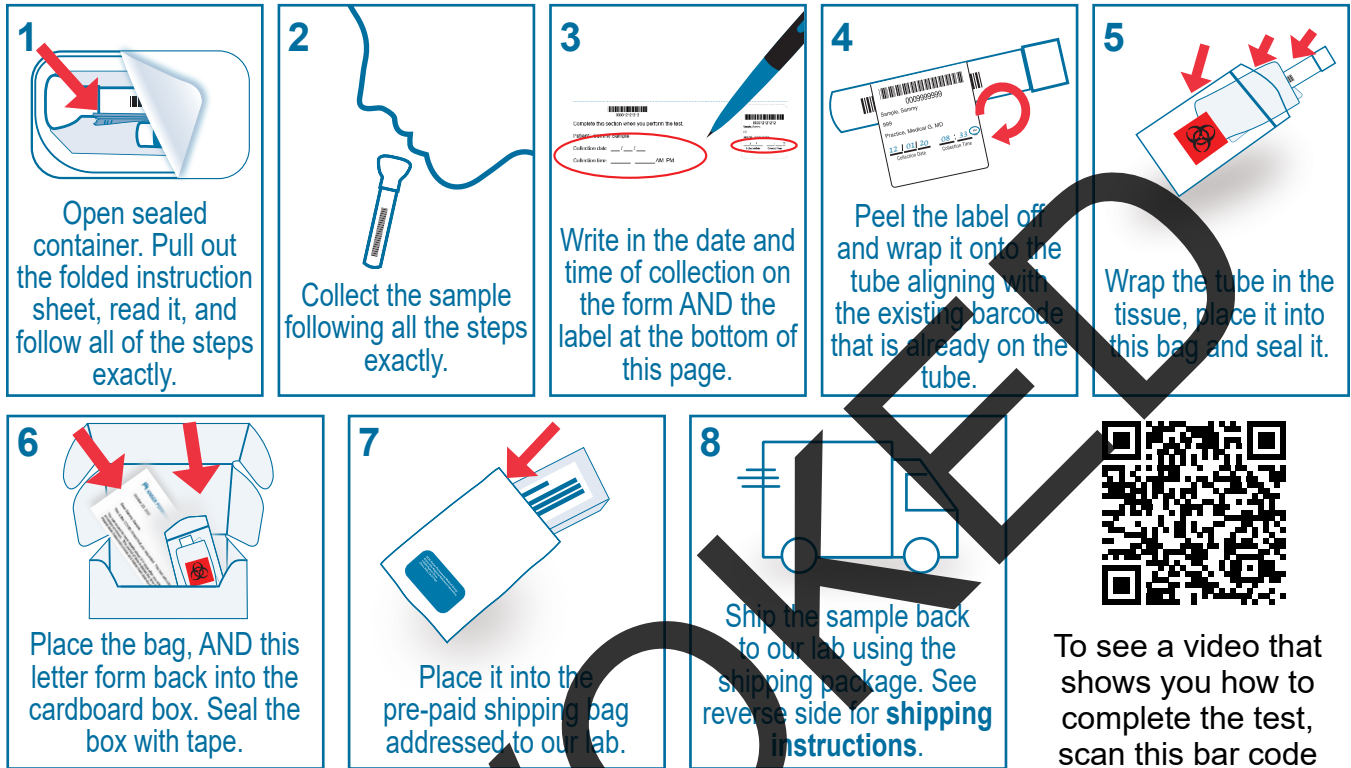

1 Open sealed container. Pull out the folded instruction sheet, read it, and follow all of the steps exactly.

2 Collect the sample following all the steps exactly.

3 Write in the date and time of collection on the form AND the label at the bottom of this page.

4 Peel the label off and wrap it onto the tube aligning with the existing barcode on the tube.

5 Wrap the tube in the tissue, place it into this bag and seal it.

6 Place the bag, AND this letter form back into the cardboard box. Seal the box with tape.

7 Place it into the pre-paid shipping bag addressed to our lab.

8 Ship the sample back to our lab using the shipping package. See reverse side for shipping instructions.

To see a video that shows you how to complete the test, scan this bar code

Please return sample back on the same day it was collected.

- This product is designed for the collection of human saliva samples.
- This product has not been FDA cleared or approved but has been authorized for emergency use by FDA under an EUA for use by SCPMG-RRL located at 13000 Peyton Drive, Chino Hills, CA 91709.
- This product has been authorized only for the detection of nucleic acid from SARS-CoV-2, not for any other viruses or pathogens.
- The emergency use of this product is only authorized for the duration of the declaration that circumstances exist justifying the authorization of emergency use of in vitro diagnostics for detection and/or diagnosis of COVID-19 under Section 564(b)(1) of the Federal Food, Drug and Cosmetics Act, 21 U.S.C. § 360bbb-3(b)(1), unless the declaration is terminated, or authorization is revoked sooner.

Please write the date and time of collection here



Complete this section after you collect the sample.

Patient: luymfu Pghhguil

Collection date: ____ / ____ / ____
mm dd yyyy

Collection time: ____ : ____ AM PM

Please write the date and time of collection here



Pghhguil, luymfu
052
.
____ / ____ / ____
mm dd yyyy
____ : ____
AM
PM



January 21, 2021

E


Dear Bcyygq,

This is the Kaiser Permanente Saliva Home Collection Kit that you requested. This test will ask you to collect a sample of your saliva. Test results are usually available on kp.org within 48 hours of when we receive your sample.

Please return the sample back to us using the pre-paid package enclosed following the shipping options on the bottom of this page. **Please return sample back on the same day it was collected. For people 18 years old and older.**

The Kaiser Permanente Saliva Home Collection Kit contents include:

- ✓ Corrugated box
- ✓ Saliva collection device with collection instructions
- ✓ Personalized patient letter with shipping instructions and label
- ✓ Biohazard bag with absorbent tissue
- ✓ Return shipping bag

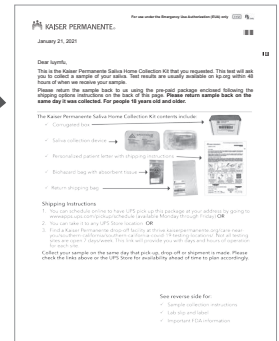

Shipping Instructions


1. You can schedule online to have UPS pick up this package at your address by going to wwwapps.ups.com/pickup/schedule (Monday through Friday) **OR**
2. You can take it to any UPS Store location Monday through Friday (go to www.ups.com/dropoff to learn more; be sure to drop off your completed kit before the latest 'Air' drop-off time) **OR**
3. Find a Kaiser Permanente drop-off facility at <https://www.kpscalfyi.org/kp-employee-and-physician-covid-19-testing/>. Not all testing sites are open 7 days/week. This link will provide you with days and hours of operation for each site.

Collect your sample (Monday through Friday) on the same day that pick-up, drop-off or shipment is made. Please check the links above ahead of time to plan accordingly.

See reverse side for:

- ✓ Sample collection instructions
- ✓ Lab slip and label
- ✓ Important FDA information

Wash hands prior to sample collection. **Do not eat, drink, smoke or chew gum for 30 minutes before providing the saliva sample.** Do not ingest the liquid in the collection device. Wash with water if liquid solution comes in contact with eyes or skin. Follow all instructions provided in the collection device for sample collection. Not following the instructions exactly can lead to incorrect results.

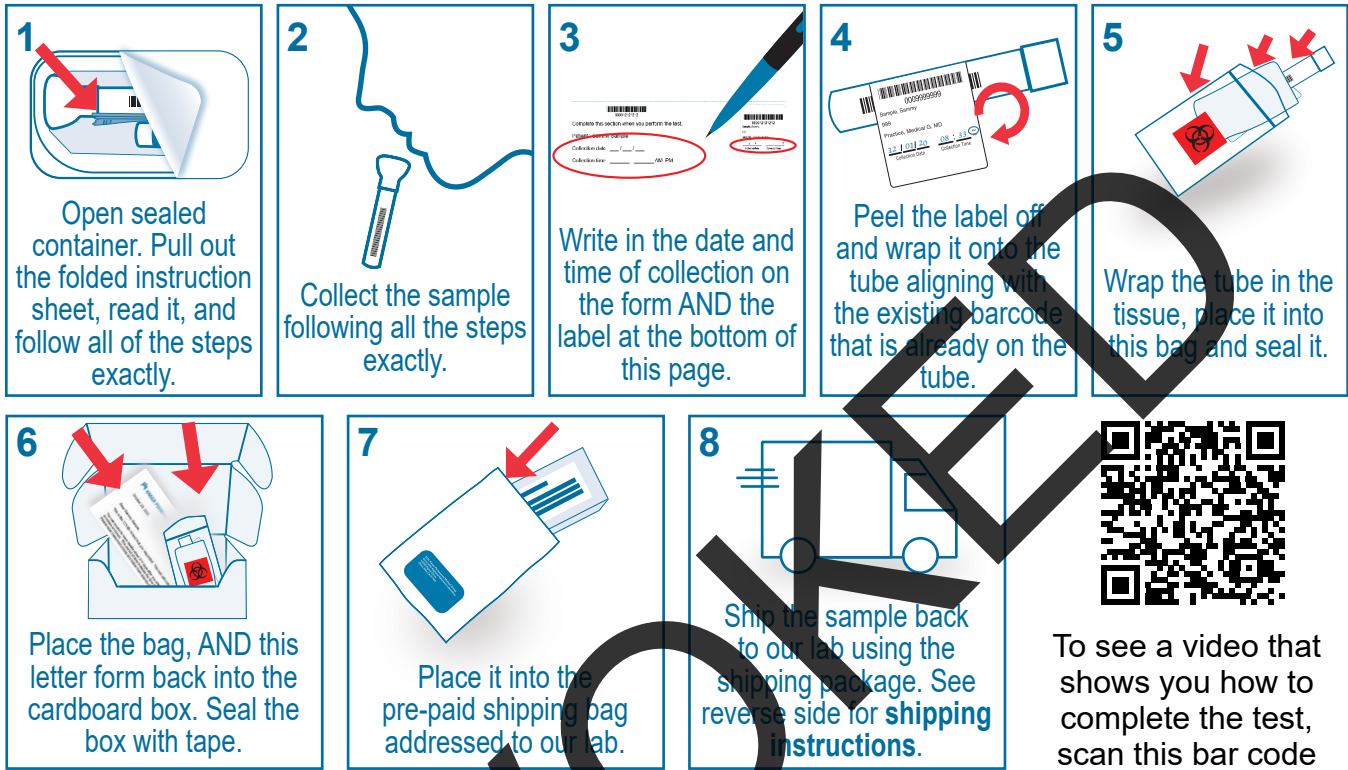

1 Open sealed container. Pull out the folded instruction sheet, read it, and follow all of the steps exactly.

2 Collect the sample following all the steps exactly.

3 Write in the date and time of collection on the form AND the label at the bottom of this page.


4 Peel the label off and wrap it onto the tube aligning with the existing barcode that is already on the tube.

5 Wrap the tube in the tissue, place it into this bag and seal it.

6 Place the bag, AND this letter form back into the cardboard box. Seal the box with tape.

7 Place it into the pre-paid shipping bag addressed to our lab.

8 Ship the sample back to our lab using the shipping package. See reverse side for shipping instructions.



To see a video that shows you how to complete the test, scan this bar code

Please return sample back on the same day it was collected.

- This product is designed for the collection of human saliva samples.
- This product has not been FDA cleared or approved but has been authorized for emergency use by FDA under an EUA for use by authorized laboratories.
- This product has been authorized only for the collection and maintenance of saliva specimens as an aid in the detection of nucleic acid from SARS CoV-2, not for any other viruses or pathogens.
- The emergency use of this product is only authorized for the duration of the declaration that circumstances exist justifying the authorization of emergency use of in vitro diagnostics for detection and/or diagnosis of COVID-19 under Section 564(b)(1) of the Federal Food, Drug and Cosmetics Act, 21 U.S.C. § 360bbb-3(b)(1), unless the declaration is terminated, or authorization is revoked sooner.

Please write the date and time of collection here



Complete this section after you collect the sample.

Patient: Bcyggq Hrpqxy

Collection date: / /
 mm dd yyyy

Collection time: : AM PM

Please write the date and time of collection here



Hrpqxy, Bcyggq
202

 / /
 mm dd yyyy
 : AM PM