
GUDID Records and Submission Compliance Dates




Data Current as of February 10, 2025





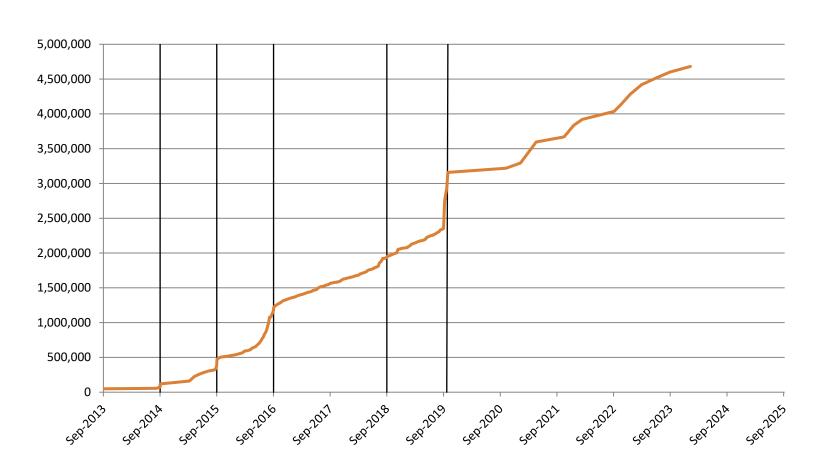


Data Current as of February 10, 2025

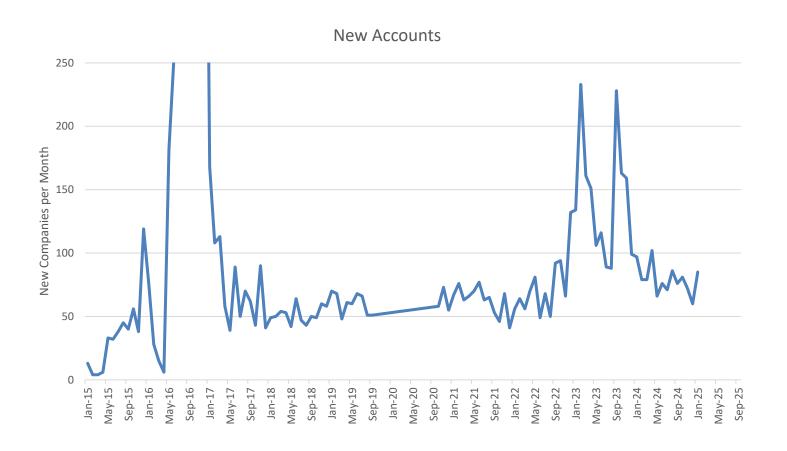

Most GUDID Records are Class II; About 31% are Associated with Implantables


"Implantable" Devices are those Assigned FDA Product Codes Associated with Implantable Devices, Systems and Accessories Data Current as of February 10, 2025

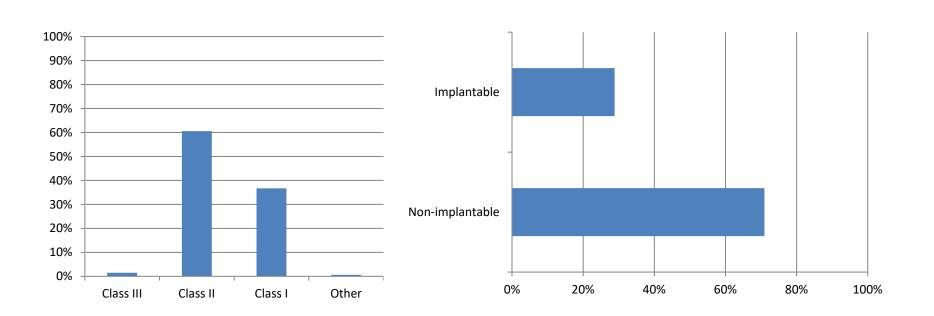

Medical Specialties in GUDID



Data Based on FDA Product Codes
Data Current as of February 10, 2025

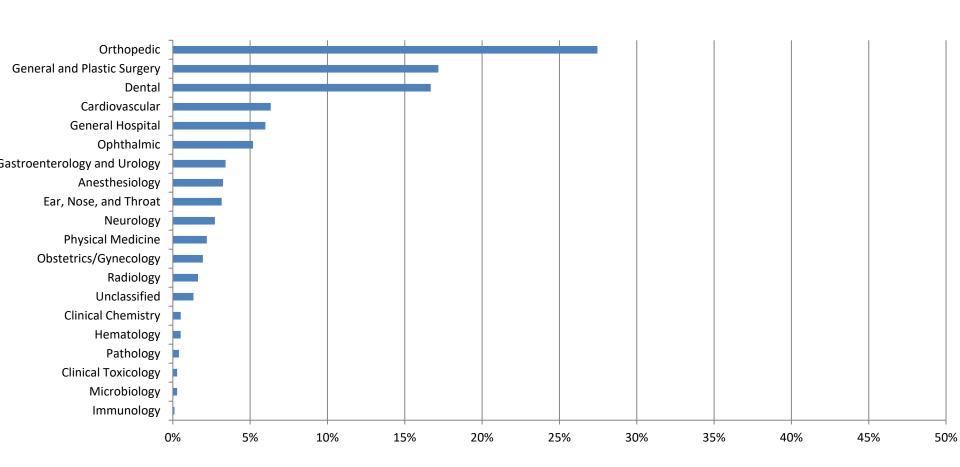

Most Frequent FDA Product Code Terms in GUDID



Data Current as of February 10, 2025

```
Blood
                                              Interlaminal Plastic Stocking Cuff
                         Cervical Use Device Replacement Aid Forceps
       Photosensitive) Coagulation Orthopedic External Scoliosis Denture Polymer/Metal/Polymer Orthosis Plate Polymer General Polymer Instrument Manual Accessories Pooling Resin Polymer Toloeps Photosensitive) Coagulation Orthopedic External Orthosis Plate Retract Polymer Hearing Abutment Porous Medical Surgery
Electrosurgical
           Sunglasses Diamond Suture Tube Spinal Screw Prevent
 Idiopathic Electrode System Fixation Support Tracheostomy
Frame Porcelain Wireless Intervertebral Metal/Polymer
Spectacle Prescription Pedicle Integrated
Spondylolisthesis Procedure Teeth Non-Porous Dental Hip Procedure Knee
                                      Bracket Semi-Constrained Adolescent Template
     Cardiovascular Implant
                                                        Lumbar Air-Conduction Graft
                            Patellofemorotibial Cutting Preformed Magnifying
                 (Non-Prescription Endosseous Body Tray


Root-Form Fusion Thoracolumbosacral

Catheter Component
```

GUDID Labeler Locations by Country



Data Current as of February 10, 2025

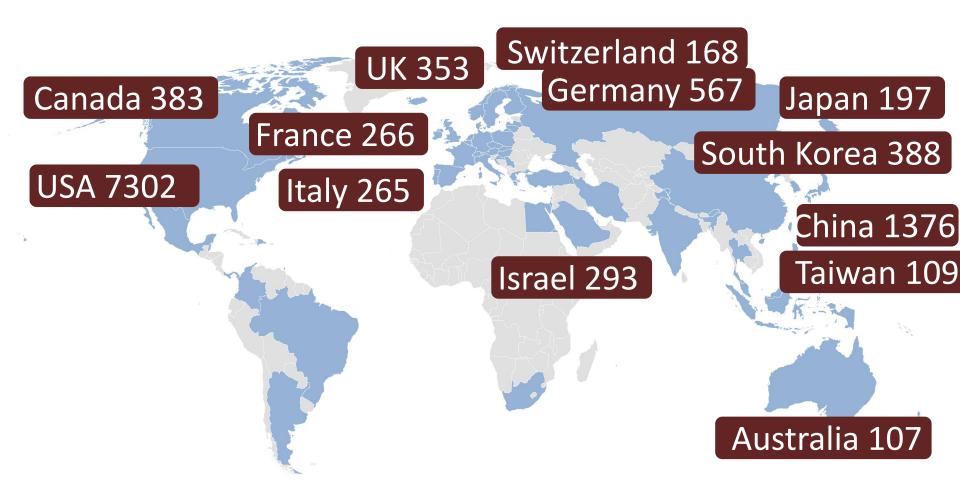

All Other Countries in Blue < 100