

Utah Medical Products, Inc.
7043 South 300 West
Midvale, UT 84047
CFN/FEI: 1718873
EI: 6/4-8/01
Thai Duong, Investigator

SUMMARY OF FINDINGS

Inspection of this medical device manufacturer was conducted as a routine DEN-DO, FY-01 workplan assignment in accordance with C.P. 7382.845, Inspection of Medical Device Manufacturers. Based on the current inspectional strategy, this inspection was conducted as a level 1 abbreviated QSIT inspection (Corrective and Preventive Action plus one additional sub system). The firm manufactures various Class II products in labor and delivery/obstetrics, neonatal intensive care, gynecology/urology/electrosurgery and blood pressure monitoring.

The previous inspection of this firm was conducted on 9/11-16/98 as a follow-up to a warning letter issued on 8/15/95. In addition, the inspection was also conducted in accordance with DEN-DO assignment, based on a request from CDRH to determine the cause of the adverse events associated with firm's Intrauterine Pressure monitors. The inspection revealed no significant deficiencies, and no FDA-483 was issued. However, a few specific GMP issues were discussed. The inspection was classified NAI.

The current inspection found the firm to have new and continuing deviations from the CGMP/QS regulation. These deviations include deficiencies in: corrective and preventive actions; device history records; process validation; non-conforming material records; electronic records and signatures; and sampling plans.

At the conclusion of the inspection, an FDA 483, Inspectional Observations, was issued to and discussed with Kevin L. Cornwell, President and CEO, as well as with John R. Smith, Quality Manager, and X X X Y, Quality Supervisor. No comments were made to the items as noted on the annotated FDA 483 and the firm promised a written response to the items within fifteen days.

Post inspectional correspondence and FMD 145 copy should be addressed to: Mr. Kevin L. Cornwell, President and CEO, Utah Medical Products, Inc., 7043 South 300 West, Midvale, UT 84047.

Sample DOC 50263 of PVC White IUP Molding Compound, IUP-400, lot # 72977, was collected to document Utah Medical Products' receipt of a component and its interstate shipment of a finished device from this facility.

HISTORY OF BUSINESS

Utah Medical Products was incorporated in the State of Utah in 1978. A copy of the 2000 Annual

Utah Medical Products, Inc.
7043 South 300 West
Midvale, UT 84047
CFN/FEI: 1718873
EI: 6/4-8/01
Thai Duong, Investigator

Report is attached as exhibit #1. The inside cover of the last page contains a listing of Board Members and Corporate Officers. The firm's Corporate Officers include: Kevin L. Cornwell, President and Secretary; Paul O. Richins, Vice President and Chief Administrative Officer; Greg A. LeClaire, Chief Financial Officer; and Mark A. Lanman, Vice President Sales.

According to the firm, the annual sales of Utah Medical Products are approximately X X X. The firm sold approximately X of the products out of the State of Utah. Utah Medical Products is currently registered with FDA as a medical device manufacturer and an initial distributor.

Utah Medical Products has X additional manufacturing facilities. The X facilities are located

X X X X X X X X X X X X
X X X X X X X X X X X X

Responsible individuals present during the inspection are as follows:

- Kevin L. Cornwell – President and CEO
- John R. Smith – Quality Manager
- X X X X – Quality Supervisor

See exhibit #2 for a copy of the firm's organizational chart.

The facility occupies a large building located at 7043 South 300 West. There currently is a total of X employees. The firm's office hours are 7:00 a.m. – 5:00 p.m., Monday through Friday. The manufacturing area operates X X X X X X X X X X X X

X X X X X X X X X X X X

The firm manufactures and offers various Class II products in labor and delivery/obstetrics, neonatal intensive care, gynecology/urology/electrosurgery and blood pressure monitoring. The products include: Fetal Monitoring (the Intrauterine Pressure (IUP) Catheters); Vacuum-Assisted Delivery systems (the Vacuum Pump and Silicon Cups); Umbilical Cord Management (the Umbilicup and Cordguard); Disposable Pressure Transducer and Blood Sampling Systems for Critical Care Monitoring (Deltran line); Electrosurgical generators (Finesse line); Gynecology Electrodes (C-LETZ Conization Electrodes); Neonatal and Pediatric Intensive Care (the Umbili-Cath, Catheterization Tray, Nutri-Cath, Myelo-Nate, Uri-Cath, Picc-Nate, Hemo-Nate, Dialy-Nate, Thora-

Utah Medical Products, Inc.
7043 South 300 West
Midvale, UT 84047
CFN/FEI: 1718873
EI: 6/4-8/01
Thai Duong, Investigator

The current inspection also covered the Intran IUP-400 product. The inspection found the firm to have new and continuing deviations from CGMP/QS regulation. See INSPECTIONAL APPROACH section below for more detail.

PERSONS INTERVIEWED & INDIVIDUAL RESPONSIBILITY

On 6/4/01, credentials were shown and FDA 482, Notice of Inspection, was issued to John R. Smith, Quality Manager, the most responsible individual at the firm by his own admission. Mr. Smith accepted the FDA 482 and introduced me to [redacted] Quality Supervisor. Mr. Smith and [redacted] accompanied me during the entire inspection and provided information and documentation for various activities.

Mr. Kevin L. Cornwell, President and CEO, was not available at the time of the issuance of the FDA 482. Mr. Cornwell was only present during the last day of the inspection to accept the FDA 483, Inspectional Observations.

On 6/8/01, an FDA 483 was issued to and discussed with Mr. Kevin L. Cornwell, as well as with Mr. John R. Smith, and [redacted] No comments were made to the items as noted on the annotated FDA 483 and the firm promised a written response to the items within fifteen days.

Mr. John R. Smith has been delegated the responsibility for quality assurance including GMP compliance since [redacted] of this year. Prior to becoming the Quality Manager, he spent [redacted] with the company as a [redacted] Mr. Smith stated that his responsibilities include management review, complaints and failure investigations, MDRs, and 510(k) submissions. He is also in charge of the Quality Group. In addition, Mr. Smith is responsible for the compliance activities for the [redacted] Mr. Smith is the firm's management representative and he reports directly to Mr. Cornwell.

[redacted] as a Quality Supervisor. She was the Quality Manager at [redacted] before joining Utah Medical Products. [redacted] is responsible for corrective and preventive action system, document control, hazardous materials, environmental monitoring, non-conforming materials, and internal audits. Mr. Smith stated that the firm hired [redacted] to help him with the quality assurance duties. She reports directly to Mr. Smith.

PURGED

Utah Medical Products, Inc.
7043 South 300 West
Midvale, UT 84047
CFN/FEI: 1718873
EI: 6/4-8/01
Thai Duong, Investigator

PROMOTION AND DISTRIBUTION

The firm ships approximately ~~X~~ of its products in interstate commerce via ~~X~~ ~~X~~ ~~X~~ ~~X~~. Promotion and distribution of the firm's products to customers are conducted through sales representative and trade shows. See exhibit #3 for the firm's promotional literatures.

SAMPLES COLLECTED

Sample DOC 50263 of PVC White IUP ~~_____~~ IUP-400, lot # 72977, was collected to document Utah Medical Products' receipt of a component and its interstate shipment of a finished device from this facility.

REFUSALS

No refusals were made.

OBJECTIONABLE CONDITIONS

The following is a listing of the items contained on the FDA 483 and any discussion regarding them.

1. Review of the firm's corrective and preventive action system revealed:

- a) Corrective and Preventive Action procedure, ~~X~~ ~~X~~, does not include the requirement for analyzing sources of quality data to identify existing and potential product and quality problems.

Discussion: The firm's Corrective/Preventive Action procedure ~~X~~ ~~X~~ Rev. ~~X~~ exhibit #7, does not address the requirement for analyzing sources of quality data to identify existing and potential product and quality problems. The procedure begins with an initiation of the corrective and preventive action request. There is no discussion of the sources of quality data to be analyzed.

- b) Not all quality data are being analyzed to identify existing and potential product and quality problems. For example: in-process rejects and MDRs.

Utah Medical Products, Inc.
7043 South 300 West
Midvale, UT 84047
CFN/FEI: 1718873
EI: 6/4-8/01
Thai Duong, Investigator

Discussion: Although the firm's Corrective/Preventive Action procedure ~~X~~ ~~X~~ Rev. ~~X~~ exhibit #7, does not include the requirement for analyzing sources of quality data, trending are being performed on certain quality data. The firm has yet to identify all sources of quality data to be analyzed to detect product and quality problems that may require corrective/preventive action.

The firm currently trends the following:

~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~

Complaint data are provided in a matrix form (see exhibit #6). The total number of complaints received is captured on a ~~X~~ ~~X~~ basis and the complaint failure codes are tracked on a ~~X~~ ~~X~~

There is no procedure addressing the above trending reports. In addition, examples of quality data not being trended include MDRs, in-process rejects, maintenance records, quality audits, etc.

At the conclusion of the inspection, Mr. Cornwell asked how does the firm determine whether they have identified all the quality data sources to be analyzed. I stated that the firm needs to look at their operations and identify the sources that provide quality data that may require corrective/preventive action. Examples of sources of quality data were given to Mr. Cornwell including the ones mentioned above.

c) There are no corrective and preventive actions taken for the problems identified in the trending reports. ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~

~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~

Discussion: The firm currently trends the following:

~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~

Utah Medical Products, Inc.
7043 South 300 West
Midvale, UT 84047
CFN/FEI: 1718873
EI: 6/4-8/01
Thai Duong, Investigator

Complaint data are provided in a matrix form (see exhibit #6). The total complaints received are captured ~~X~~ ~~X~~ and the complaint failure codes are tracked on a ~~X~~ ~~X~~ ~~X~~

Although the above analysis reports identified unfavorable trends and problem areas, there are no documented evidence showing that any corrective or preventive actions have been taken to directly address the identified issues. ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~

~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~

2. Review of the firm's Device History Records (DHRs) for the Intran Plus Catheters, IUP-400 revealed the following:

a) Manufacturing Procedure ~~X~~ ~~X~~ Intran Plus and IUP-300 Final Tester, does not assure that IUP catheters conform to all approved design specifications prior to acceptance. Device Master Record specifications for Unbalance are ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ release of finished devices in the range of ~~X~~ ~~X~~ ~~X~~ ~~X~~

Discussion: The Device Master Record for the Intran Sensor Tipped Catheters, IUP-400, is attached as exhibit #9. The sensor specifications for Unbalance are ~~X~~ ~~X~~ ~~X~~ ~~X~~

A copy of Manufacturing Procedure ~~X~~ ~~X~~ Intran Plus and IUP-300 Final Tester, is attached as exhibit #10. ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~

~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ Although it is not mentioned in the procedure, the final test is performed by ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ The individual test results are

~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~


~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ ~~X~~ The Summary Report for each lot is included with the Device History Record.

Review of the Device History Records, exhibit #12, revealed the specifications set for Unbalance are ~~X~~ ~~X~~ ~~X~~ By following this procedure, the firm can accept a catheter with an Unbalance between ~~X~~ ~~X~~ ~~X~~ which does not meet DMR specifications of ~~X~~ ~~X~~ ~~X~~


In the Summary Report, the firm no longer prints out the graphs of the results obtained from the

Utah Medical Products, Inc.
7043 South 300 West
Midvale, UT 84047
CFN/FEI: 1718873
EI: 6/4-8/01
Thai Duong, Investigator

tests. However, some of the DHRs in year ~~X~~ do contain the summary graphs. The DHRs can be reviewed for the following information:

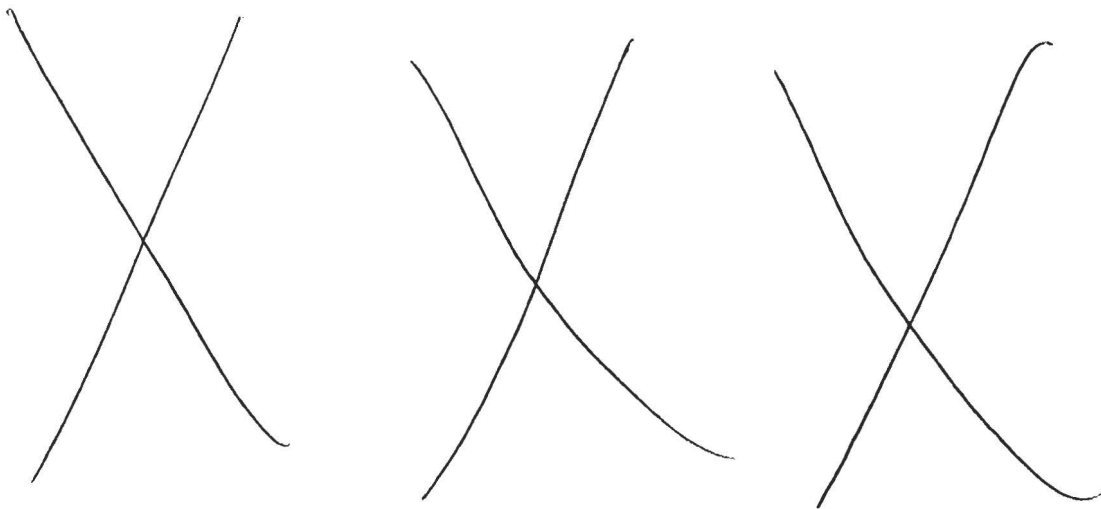

Discussion: A copy of the Work Order Traveler/Bill of Operations is attached as exhibit #11. The Work Order Traveler lists the various operations need to be performed. This include the following required tests:

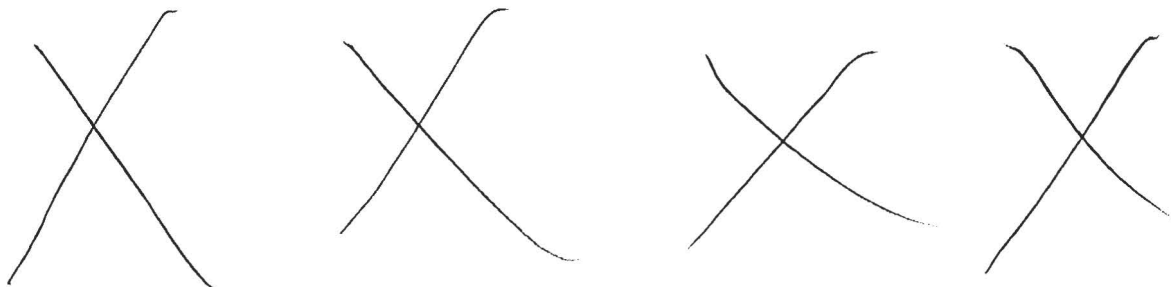

Utah Medical Products, Inc.
7043 South 300 West
Midvale, UT 84047
CFN/FEI: 1718873
EI: 6/4-8/01
Thai Duong, Investigator

X X X X X X X X X X X X

Review of the DHRs, exhibit #12, revealed that there are no documented evidence showing that the above tests are being performed. The Work Order Operation Tracking Form procedure, exhibit #18, requires the above tests be documented on the tracking form once the test is completed, but it allows the form to be discarded at packaging.

According to the firm, the purpose of the form is to allow the operators at packaging to verify that the tests were performed. Once the form is verified, the operator can get rid of it. I stated that I also need to know whether these required tests were performed, and the only way I can tell is by looking at the documentation.

c) Not all rejects are identified and documented. The devices failed during final test, documented in the Intran Plus Final Tester Summary Report, does not indicate its final disposition.

Discussion: Review of the firm's IUP-400 DHRs, exhibit #12, revealed that not all rejects from the lot are identified and documented. Specifically, the rejects from the required tests cited in the above item (2b).

Although the above tests are documented on the tracking form, the form does not include the quantity sampled, the quantity passed, and the quantity failed from each test. An example of the tracking form is attached as exhibit #19. In addition, examples from the DHRs collected to demonstrate the observation are as follow:

X X X X X
X X X X X

PURGED

Utah Medical Products, Inc.
7043 South 300 West
Midvale, UT 84047
CFN/FEI: 1718873
EI: 6/4-8/01
Thai Duong, Investigator

(exhibit #22.4).

During the inspection, X X stated that the firm was having problems with printing out an incoming inspection record. Nevertheless, the firm was able to provide an example of the incoming inspection record from their computer system. A copy of the incoming inspection record is attached as exhibit #23.

6. For the electronic records and signatures, there are no procedures addressing the following:

- a) Validation of systems to ensure accuracy, reliability, consistent intended performance, and the ability to discern invalid or altered records.
- b) The ability to generate accurate and complete copies of records.
- c) Protection of records throughout the record retention period.
- d) Limiting system access.
- e) And the system can create an audit trail that is computer-generated, time stamped to independently record the date and time of operator entries and actions.

Discussion: Electronic records and signatures are being used in the complaint and incoming inspection systems. The firm lacks procedures to address the requirements for electronic records and signatures set forth in 21 CFR Part 11.

Mr. Smith was not aware of the requirements in Part 11. He stated that the firm needs to look at the requirements for electronic records and signatures and see whether they can comply.

7. Sampling plans used are not always based on a valid statistical rationale. For example:

X - X X X X X X X

Discussion: The firm's sampling plans for incoming inspections and in-process testing are not always based on a valid statistical rationale. For example:

Utah Medical Products, Inc.
7043 South 300 West
Midvale, UT 84047
CFN/FEI: 1718873
EI: 6/4-8/01
Thai Duong, Investigator

Incoming inspection procedure for Introducer, Break Away Needle, Metal, 2 French (Yellow), exhibit #24, requires inspection of ~~7~~ units for the various criteria regardless of lot size.

In-process inspection procedure for _____, exhibit #14, requires checking ~~7~~ ~~8~~ ~~9~~ to ensure that the _____

DISCUSSION WITH MANAGEMENT

At the conclusion of the inspection, an FDA 483 was issued to and discussed with Mr. Kevin L. Cornwell, CEO, as well as with Mr. John R. Smith, Quality Manager, and ~~7~~ ~~8~~ ~~9~~ Quality Supervisor. No comments were made to the items as noted on the annotated FDA 483 and the firm promised a written response to the items within fifteen days.

Mr. Cornwell was informed that these items were not all inclusive and the firm is responsible for conducting audits and correcting any and all violations of the CGMP/QS regulation. I advised Mr. Cornwell of the sanctions available to FDA if corrections are not made, including warning letter, seizure, injunction, and prosecution.

ATTACHMENTS:

FDA-482 issued
FDA-483 issued


EXHIBITS:

1. 2000 Annual Report
2. Organizational Chart
3. Product Catalogs
4. 510(k) Listing
5. Facility Floor Plans
6. Complaint Matrices
7. Corrective/Preventive Action Procedure
8. Trending Reports
9. Device Master Record for Intran Sensor Tipped Catheters

PURGED

Utah Medical Products, Inc.
7043 South 300 West
Midvale, UT 84047
CFN/FEI: 1718873
EI: 6/4-8/01
Thai Duong, Investigator

10. Intran Plus and IUP-300 Final Tester Procedure - X X
11. Bill of Operations – IUP-400 Intran Plus
12. IUP-400 Device History Records
13. Testing Tubing for Leaks Procedure - X X
14. Thread Wire Though Housing and Tubing Procedure - X X
15. Intran Plus Switch Plus Procedure - X X
16. Overmold Primer Application Procedure - X X
17. Overmold Process Procedure - X X
18. Work Order Operation Tracking Form Procedure
19. Work Order Operation Tracking Form
20. Non-Conforming Materials Procedure - _____
21. Non-Conforming Materials Reports
22. Complaint Report
23. Incoming Inspection Record
24. Incoming Inspection Procedure - Introducer, Break Away Needle, Metal, 2 French

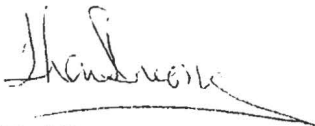

Thai Duong,
Investigator

PURGED FOR HRMS USE ONLY